



Heriot-Watt University  
Research Gateway

## Microfluidics for effective concentration and sorting of waterborne protozoan pathogens

### Citation for published version:

Jimenez, M & Bridle, H 2016, 'Microfluidics for effective concentration and sorting of waterborne protozoan pathogens', *Journal of Microbiological Methods*, vol. 126, pp. 8-11.  
<https://doi.org/10.1016/j.mimet.2016.04.008>

### Digital Object Identifier (DOI):

[10.1016/j.mimet.2016.04.008](https://doi.org/10.1016/j.mimet.2016.04.008)

### Link:

[Link to publication record in Heriot-Watt Research Portal](#)

### Document Version:

Peer reviewed version

### Published In:

Journal of Microbiological Methods

### General rights

Copyright for the publications made accessible via Heriot-Watt Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

### Take down policy

Heriot-Watt University has made every reasonable effort to ensure that the content in Heriot-Watt Research Portal complies with UK legislation. If you believe that the public display of this file breaches copyright please contact [open.access@hw.ac.uk](mailto:open.access@hw.ac.uk) providing details, and we will remove access to the work immediately and investigate your claim.

## Accepted Manuscript

Microfluidics for effective concentration and sorting of waterborne protozoan pathogens

M. Jimenez, H. Bridle

PII: S0167-7012(16)30068-9  
DOI: doi: [10.1016/j.mimet.2016.04.008](https://doi.org/10.1016/j.mimet.2016.04.008)  
Reference: MIMET 4875

To appear in: *Journal of Microbiological Methods*

Received date: 29 March 2016  
Revised date: 7 April 2016  
Accepted date: 7 April 2016



Please cite this article as: Jimenez, M., Bridle, H., Microfluidics for effective concentration and sorting of waterborne protozoan pathogens, *Journal of Microbiological Methods* (2016), doi: [10.1016/j.mimet.2016.04.008](https://doi.org/10.1016/j.mimet.2016.04.008)

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

**REVISION**

Microfluidics for Effective Concentration and Sorting of Waterborne Protozoan Pathogens

Jimenez, M. and Bridle, H.

Institute of Biological Chemistry, Biophysics and Bioengineering

Heriot-Watt University, Riccarton, Edinburgh, EH14 4AS, Scotland

**Abstract:** We report on an *inertial focussing based* microfluidics technology for concentrating waterborne protozoa, achieving a 96% recovery rate of *Cryptosporidium parvum* and 86% for *Giardia lamblia* at a throughput (mL/min) capable of replacing centrifugation. The approach can easily be extended to other parasites and also bacteria.

Microfluidics has been proposed for the sample processing and monitoring of waterborne pathogens, with a greater emphasis in previous work being placed on the detection stages [1]. Some microfluidics waterborne pathogen sample processing has been demonstrated, e.g. on-chip immunomagnetic separation [2], electrical methods of pathogen isolation [3, 4] and on-chip filtration [5-7], although sample volumes have remained relatively small [8, 9]. By appropriate design of channel geometries high-throughput particle concentration and sorting can be achieved in microfluidics without the use of any labels, electrical fields or in-channel constrictions [10]. One such technique is known as inertial focussing [11-13] (Figure 1a) and here we report on the use of spiral channel inertial focussing microfluidics for the effective concentration of waterborne protozoa.

Devices were designed using AutoCAD and manufactured by Epigem in Epoxy and PMMA with a channel width of 170 $\mu$ m and a height of 30 $\mu$ m with four sample outlets (Figure 1b). The system was operated at flow rates between 200 and 1500 $\mu$ L/min using a mid-pressure syringe pump (neMESIS, Cetoni, GmbH). We have previously characterised the behaviour of a similar system with just two outlets using polystyrene beads (Magsphere Inc, USA) and shown that this system could also work successfully at 400 $\mu$ L/min with *Cryptosporidium parvum* (Waterborne Inc, USA) without notable impact on the viability of this pathogen [14].

Here we report on the use of a four outlet system with both *Cryptosporidium parvum* and *Giardia lamblia* (Waterborne Inc; spiked at a concentration of 1million (oo)cysts/mL) in deionised water (tap water samples have also been tested proving that the system is capable of handling these without clogging) at high flow rates (up to 1500 $\mu$ L/min), achieving a four-fold concentration with just one passage through the system. The behaviour of the pathogens within the flow channel has been analysed using a high-speed camera (CCD ProgRes, Jenoptik, GmbH on a Nikon, x 10 or x 25 magnification, inverted microscope) to image particle trajectories within the channel. Additionally, the recovery rates have been determined by counting the number of pathogens in each outlet; *from a few hundred image per outlets, taken during system operation, pathogens are counted, to a total of at least 1000, using thresholds based on intensity differences between the background and pathogens with a MATLAB script.*

Figure 1A illustrates the principle of inertial focussing in a spiral channel showing how the forces acting on particles within the flow result in them adopting laterally focussed positions, in general closer to the inner wall of the spiral. Figure 1B shows the particular device utilised within this work. By focussing pathogens into a particular location, with appropriate design of the channel geometry, pathogens can be concentrated and separated by direction to a particular outlet channel. A four outlet device achieves a concentration factor of four which can easily be increased by recirculation of the output of the appropriate outlet through the device until the desired concentration is reached (*with a stacked system we have concentrated 40mL to 0.5mL in less than 10 mins*). An alternative would be to increase the number of outlets. Here, however, we have focussed on the behaviour of waterborne protozoa within a spiral channel, which has not been previously studied. Evidently, understanding the pathogen behaviour is essential information to inform accurate and appropriate outlet positioning. The focussing behaviour of pathogens is expected to vary from that of rigid spherical particles (on which the inertial focussing theory is developed) due to their non-uniform shape and their deformability. *Cryptosporidium parvum* is approximately 4.5 by 5.5 $\mu\text{m}$  [15] and the deformability has recently been analysed with FluidFM [16]. *Giardia lamblia* cyst is approximately 10 to 20 $\mu\text{m}$  in length, 7-10 $\mu\text{m}$  in width and 0.3-0.5 $\mu\text{m}$  thickness [17, 18].

Figure 2 shows how the channel focussing location of protozoa varies with flow rate in comparison to polystyrene beads of similar sizes. It is clear that the focussing positions of *Cryptosporidium* and *Giardia* are similar to that of 5.2 and 10.3 $\mu\text{m}$  rigid particles, respectively as might be expected from their sizes. However, particularly for *Giardia* the distribution of the focussed pathogens is wider than that of the respective beads, probably due to a greater size distribution in the pathogen population, or an impact of being non-spherical and deformable, compared to the particles: for a flowrate of 500 $\mu\text{L}/\text{min}$ , 10.3 $\mu\text{m}$  beads present a standard deviation in their averaged lateral position of 8  $\mu\text{m}$  while *Giardia* is at 24  $\mu\text{m}$  (15 $\mu\text{m}$  for *Cryptosporidium*). *This difference in distribution might be explained by greater non-uniformity in the Giardia shape compared to Cryptosporidium oocysts, or deformability differences between the pathogens although data is not available to easily compare the relative deformability.*

In addition to effective high-throughput processing, recovery rate of protozoa is a critical factor for waterborne pathogen monitoring applications. Figure 3 illustrates the recovery rates of pathogens into the different outlets at different flow rates. 95% of *Cryptosporidium*, a rate comparable to that achieved in traditional IMS [5], is collected in outlet 4 at a flow rate of 1000 $\mu\text{L}/\text{min}$  demonstrating a higher recovery rate than that demonstrated for *Giardia* (86% to outlet 4 at 1500 $\mu\text{L}/\text{min}$ ) probably due to the narrower size distribution observed for this pathogen.

It can also be noted that the focussing position of the *Giardia* is closer to the centreline (Figure 2), as would be expected for a biological deformable particle [19]. However, *Cryptosporidium* does not display this trend perhaps suggesting it is less deformable or that the results for *Giardia* are actually due to the highly irregular shape of this pathogen. The *Cryptosporidium* data indicates that the pathogen focussing position initially moves towards the inner wall as flow rates increase until a limit of 700  $\mu\text{L}/\text{min}$  and further flow rate increases push the pathogen further and further back towards the centreline (Figure 2). This phenomenon has been previously observed for small particles [20], and indicates the importance of flow rate optimisation for this method to effectively concentrate pathogens. The flow rate must be selected to successfully focus all pathogens within the collection zone of a particular outlet as opposed to spreading them across two or more outlets. Additionally,

the flow rate can be manipulated to control whether simultaneous collection of both pathogens or separation of them can be achieved, e.g. as flow rates increase *Giardia* is increasingly found in outlet D whereas *Cryptosporidium* moves to being mainly collected in outlet C (Figure 3).

In conclusion, we have shown how inertial focussing microfluidics can be applied for the high-throughput concentration and separation of waterborne protozoa. By imaging the behaviour of pathogens within the channel at mL/min flow rates we have shown how this system concentrates protozoa into particular collection outlets. Therefore, the microfluidic system is capable of incorporation into existing protozoan monitoring processes: further scale-up by stacking of devices can enable processing of 50mL in less than 10 mins, and recirculation can increase the extent of concentration achieved; thus the use of microfluidics instead of centrifugation is now a feasible proposition. This could enable automation of the final stages of waterborne protozoa monitoring into an on-chip technology incorporating this concentration method with on-chip detection technologies. Furthermore, the approach can easily be adapted for other parasites or bacteria through simple modification of channel geometries.

#### Acknowledgements

M.J. and H.B. would like to acknowledge EU funding for the project "AQUAVALENS: protecting the health of Europeans by improving methods for the detection of pathogens in drinking water and water used in food preparation" and the EPSRC Impact Acceleration Award. H.B. would like to acknowledge The Royal Academy of Engineering/EPSRC for her research fellowship. M.J. and H.B. would like to acknowledge Epigem for the manufacturing part and Brian Miller for design considerations of inertial focussing devices in this type of application.

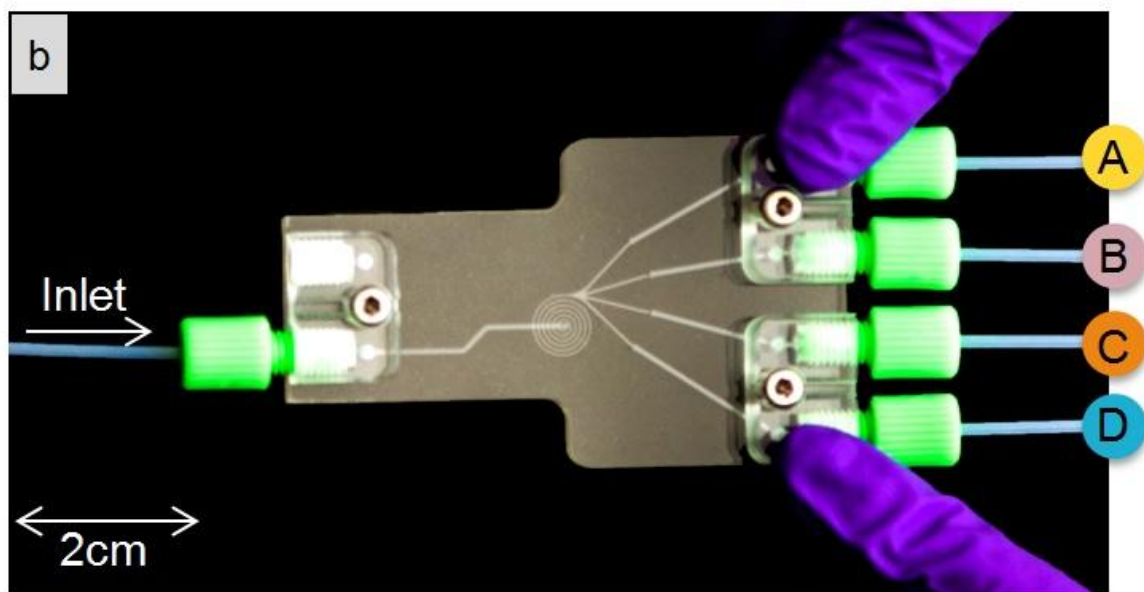
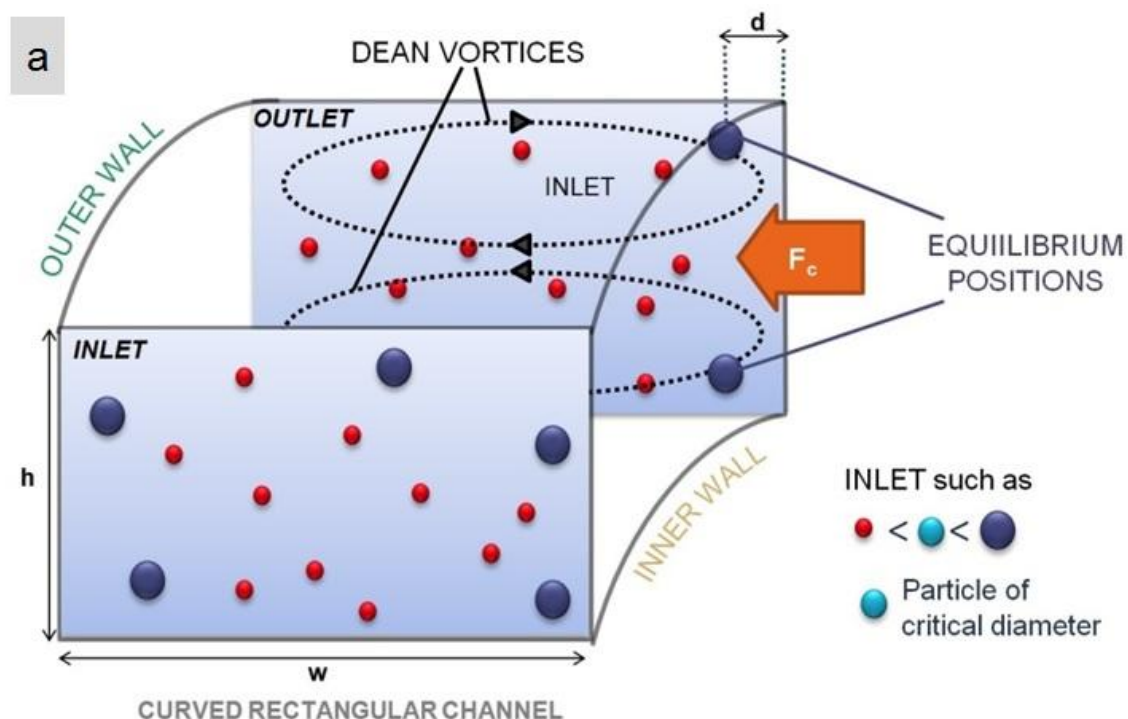


Figure 1: a) The schematic illustrates the principle of inertial focussing whereby the interplay of different forces within the flow channel act to locate particles at a particular channel location perpendicular to the flow direction (this is known as the focussing position and is typically closer to the inner wall of a spiral channel). The effect is dependent upon flow rate and particle size and deformability and  $F_c$  denotes the centrifugal action acting on the liquid towards the outer wall. Further details can be found in [11-13] ; b) The image illustrates the set-up and the size of the microfluidic device. This system can focus particles  $\leq 2 \mu\text{m}$ . More details about the design of the spiral are available in [14].

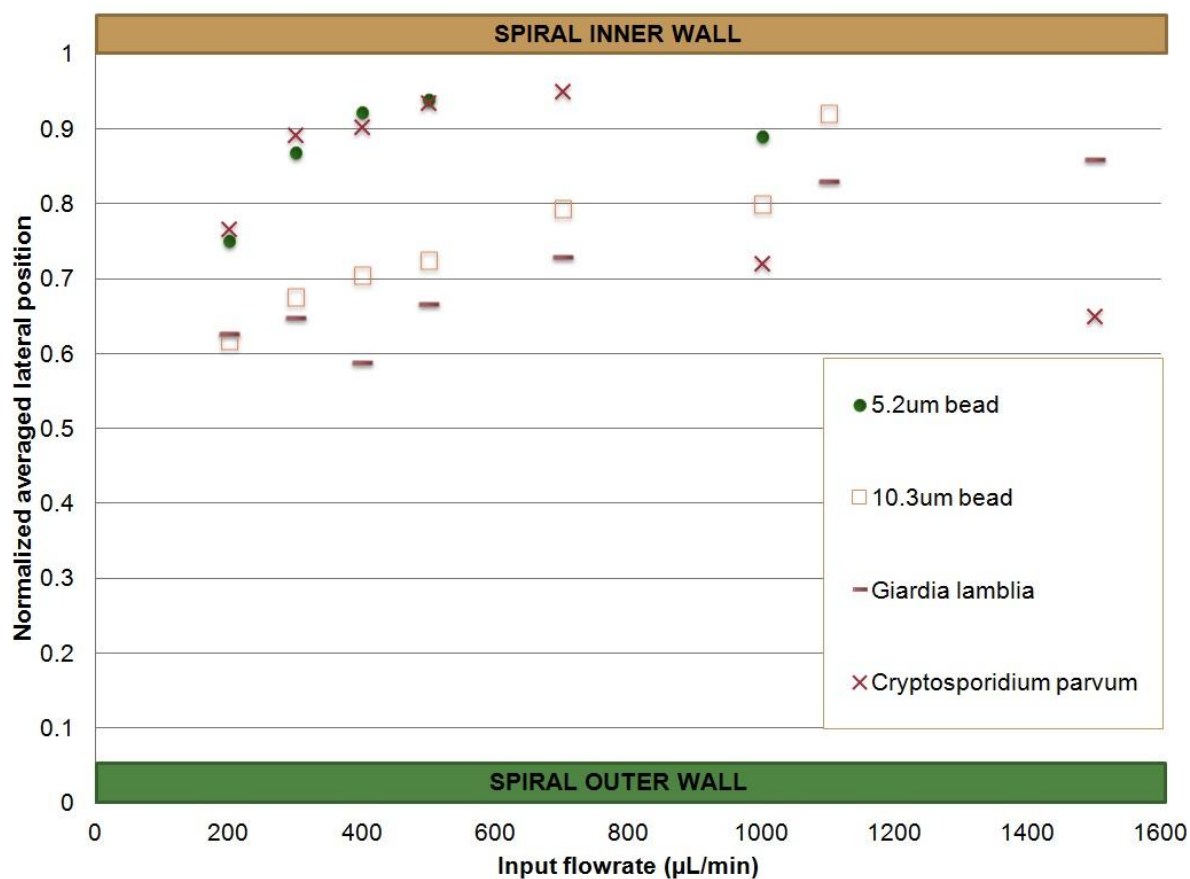


Figure 2: Focussing positions of the protozoan pathogens as compared to rigid polystyrene beads at different flow rates. The normalized averaged lateral position corresponds to  $d/w$  (distance from *outer* wall/channel width), notation as shown in Figure 1.

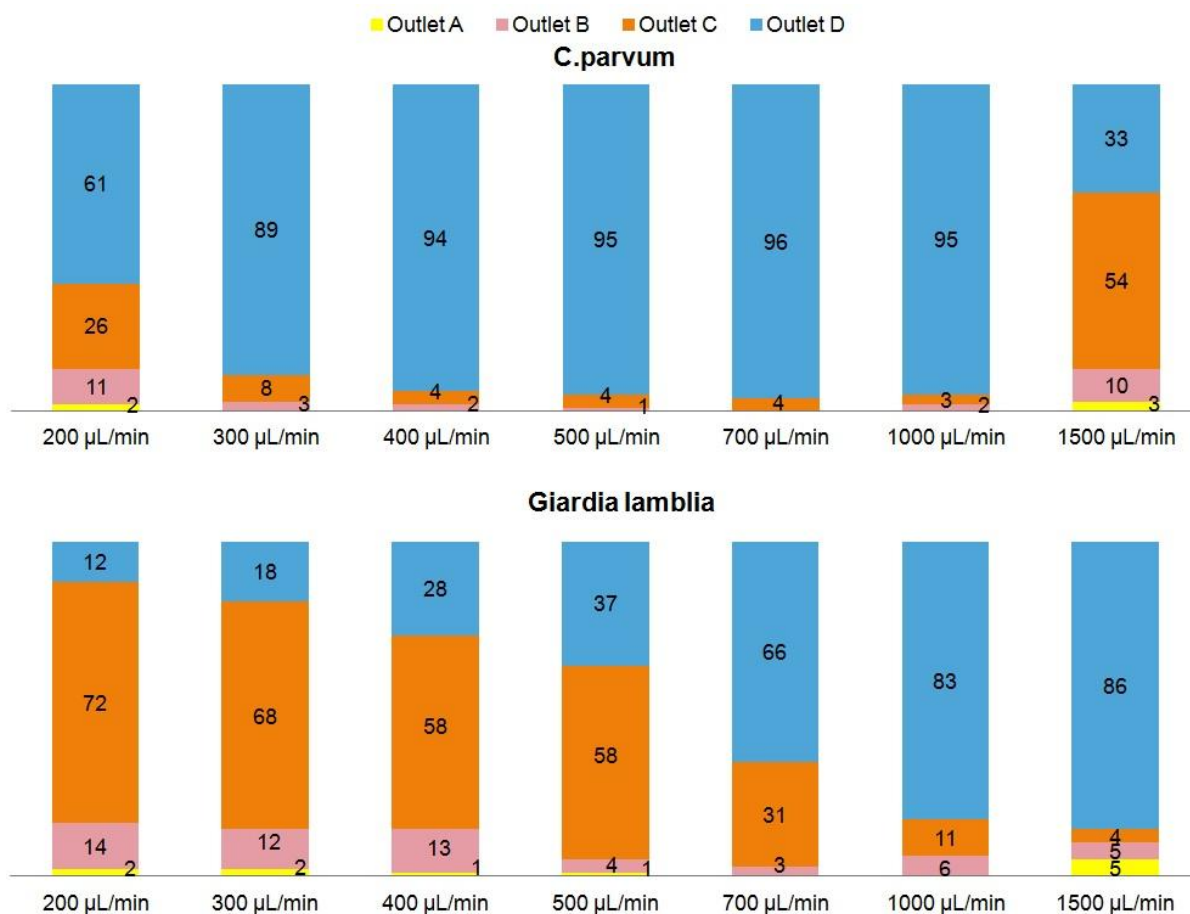


Figure 3: Recovery rates into the different outlets achieved for *Cryptosporidium parvum* and *Giardia lamblia* at different flow rates. The colour coding in the images corresponds to the different outlet colour-coding as shown in Figure 1. The percentage of pathogens found in each outlet at the different flow rates is shown, indicating the flow rate at which maximal recovery rates into one outlet can be achieved, i.e. into outlet D 0.7mL/min for *Cryptosporidium* at 96% and 1.5mL/min for *Giardia* at 86%.



## References

1. Bridle, H., *Chapter Ten - Miniaturized Detection Systems*, in *Waterborne Pathogens*. 2014, Academic Press: Amsterdam. p. 319-348.
2. Ramadan, Q., et al., *Flow-through immunomagnetic separation system for waterborne pathogen isolation and detection: Application to Giardia and Cryptosporidium cell isolation*. *Analytica Chimica Acta*. **673**(1): p. 101-108.
3. Goater, A.D., J.P.H. Burt, and R. Pethig, *A combined travelling wave dielectrophoresis and electrorotation device: applied to the concentration and viability determination of Cryptosporidium* *J. Phys. D: Appl Phys*, 1997. **30**: p. L65-L69.
4. Simmons, B.A., et al., *Concentration and separation of biological organisms by ultrafiltration and dielectrophoresis*. 2010, Sandia Corporation: U.S.
5. Taguchi, T., H. Takeyama, and T. Matsunaga, *Immuno-capture of Cryptosporidium parvum using micro-well array*. *Biosensors and Bioelectronics*, 2005. **20**: p. 2276-2282.
6. Taguchi, T., et al., *Detection of Cryptosporidium parvum oocysts using a microfluidic device equipped with the SUS micromesh and FITC-labeled antibody*. *Biotechnology and Bioengineering*, 2007. **96**(2): p. 272-280.
7. Lay, C., et al., *Enhanced microfiltration devices configured with hydrodynamic trapping and a rain drop bypass filtering architecture for microbial cells detection*. *Lab on a Chip*, 2008. **8**(5): p. 830-833.
8. Bridle, H., B. Miller, and M.P.Y. Desmulliez, *Application of microfluidics in waterborne pathogen monitoring: A review*. *Water Research*, 2014. **55**: p. 256-271.
9. Bridle, H., et al., *Detection of Cryptosporidium in miniaturised fluidic devices*. *Water Research*, 2012. **46**(6): p. 1641-1661.
10. Wyatt Shields Iv, C., C.D. Reyes, and G.P. Lopez, *Microfluidic cell sorting: a review of the advances in the separation of cells from debulking to rare cell isolation*. *Lab on a Chip*, 2015. **15**(5): p. 1230-1249.
11. Zhang, J., et al., *Fundamentals and applications of inertial microfluidics: a review*. *Lab on a Chip*, 2016. **16**(1): p. 10-34.
12. Martel, J.M. and M. Toner, *Inertial Focusing in Microfluidics*. *Annual review of biomedical engineering*, 2014. **16**: p. 371-396.
13. Di Carlo, D., *Inertial microfluidics*. *Lab on a Chip*, 2009. **9**(21): p. 3038-3046.
14. Jimenez, M., B. Miller, and H.L. Bridle, *Efficient separation of small micro particles at high flowrates using spiral channels: application to waterborne pathogens*. *Chemical Engineering Science*.
15. Smith, H.V. and R.A.B. Nichols, *Cryptosporidium: detection in water and food*. *Experimental Parasitology*, 2010. **124**: p. 61-79.
16. McGrath, J.S., et al., *Deformability Assessment of Waterborne Protozoa Using a Microfluidic-Enabled Force Microscopy Probe*. *PLoS ONE* 2016. **11**(3): p. e0150438.
17. Huang, D.B. and A.C. White, *An Updated Review on Cryptosporidium and Giardia*. *Gastroenterology Clinics of North America*, 2006. **35**(2): p. 291-314.
18. Krauss, H., et al., *Parasitic Zoonoses. Zoonoses: Infectious Diseases Transmissible from Animals to Humans (3rd ed.)* 2003, Washington D.C.: ASM Press.
19. Hur, S.C., et al., *Deformability-based cell classification and enrichment using inertial microfluidics*. *Lab on a Chip*, 2011. **11**(5): p. 912-920.
20. Martel, J.M. and M. Toner, *Particle Focusing in Curved Microfluidic Channels*. *Scientific Reports*, 2013. **3**: p. 3340.

**HIGHLIGHTS**

Microfluidics for Effective Concentration and Sorting of Waterborne Protozoan Pathogens

Jimenez, M. and Bridle, H.

Institute of Biological Chemistry, Biophysics and Bioengineering

Heriot-Watt University, Riccarton, Edinburgh, EH14 4AS, Scotland

- Concentration of parasites with a 96% recovery rate at 1.5mL/min using microfluidics
- Cryptosporidium and Giardia can be separated or jointly concentrated, depending on device operation
- Inertial focussing microfluidics could process 50mL in less than 10 mins