



Heriot-Watt University
Research Gateway

Increased Sensitivity of Long Period Grating Hydrogen Sensors Through Coupling to Higher Order Cladding Modes

Citation for published version:

Carter, R, Maier, RRJ, Biswas, P, Bandyopadhyay, S, Basumallick, N, Jones, B, McCulloch, S & Barton, J 2012, 'Increased Sensitivity of Long Period Grating Hydrogen Sensors Through Coupling to Higher Order Cladding Modes', 22nd International Conference on Optical Fiber Sensors, Beijing, China, 15/10/12 - 19/10/12.

Link:

[Link to publication record in Heriot-Watt Research Portal](#)

Document Version:

Peer reviewed version

General rights

Copyright for the publications made accessible via Heriot-Watt Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

Heriot-Watt University has made every reasonable effort to ensure that the content in Heriot-Watt Research Portal complies with UK legislation. If you believe that the public display of this file breaches copyright please contact open.access@hw.ac.uk providing details, and we will remove access to the work immediately and investigate your claim.

1. Motivation


Reliable hydrogen detection technologies required for safety applications

- Hydrogen often suggested as future fuel source
- Hydrogen explosive at 4 - 97% in air
- Most systems based on the absorption of hydrogen in palladium
- Optical system preferable for safety reasons
 - No heating
 - No electrical currents
- LPG based hydrogen sensors demonstrated
 - Low responsivity
 - High order modes are more sensitive
- Increase in responsivity leads to decreased equipment cost/requirements
- AWE have a specific requirement:
 - Long term monitoring (>10yrs)
 - Hostile environment
 - Low hydrogen concentrations (<1.5%)
 - Long term fluctuations
 - Remote monitoring system
 - Selective to hydrogen
- Optical solution is preferred

2. Palladium (Pd) - Hydrogen

Palladium absorbs hydrogen readily

- Molecular hydrogen is dissociated on Pd surface
- Atomic hydrogen then absorbed into the lattice
- Hydrogen sits in interstitial lattice sites
- Essentially a non bonding process
- Provides a strain on the lattice
- Strain alters the electron bonds
- Gives a small change in refractive index

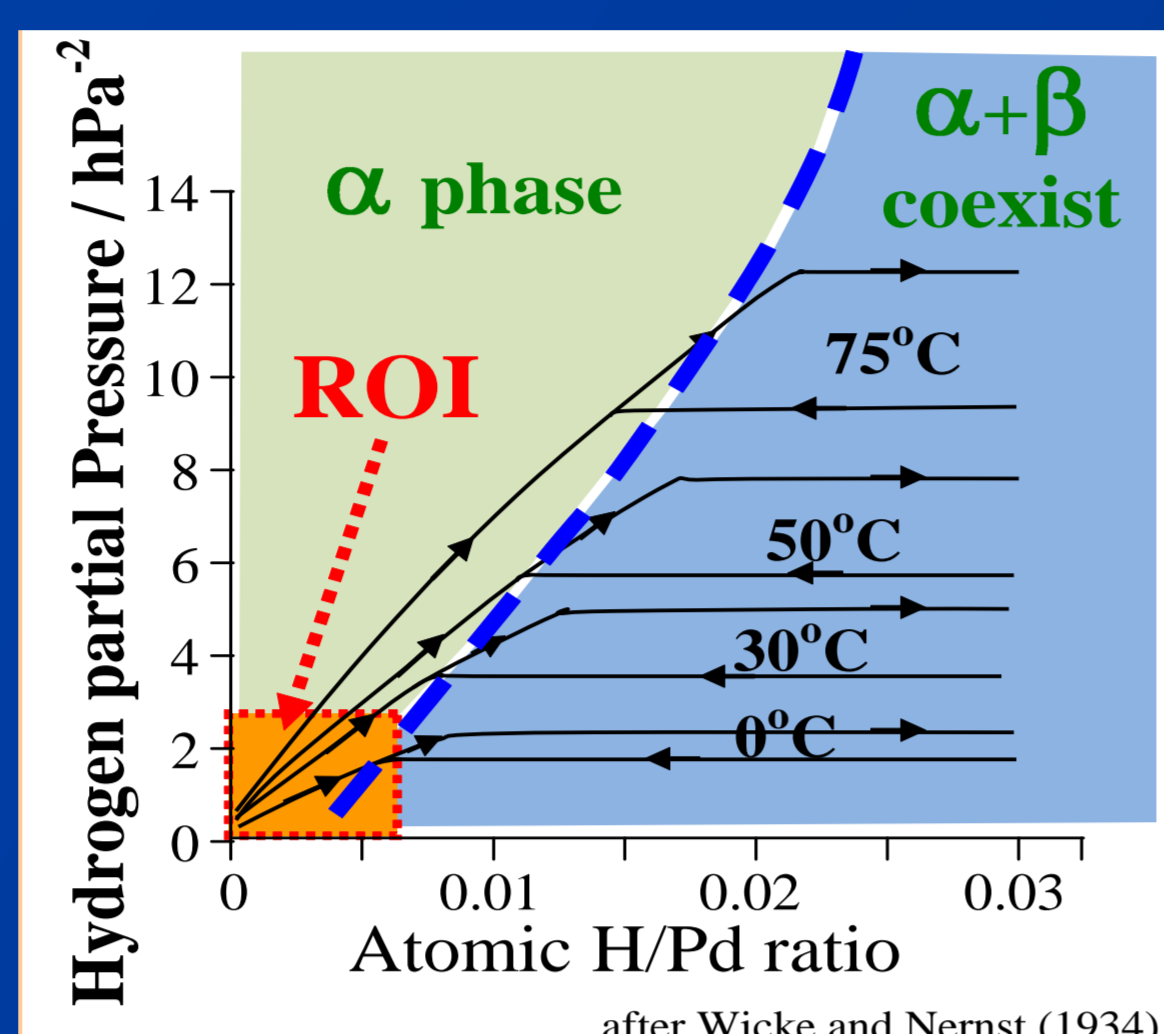


- At low concentrations (<4%) process is reversible
- At higher concentrations lattice phase shift proves destructive
- Most sensor systems based on the absorption of hydrogen in palladium


3. Long Period Gratings

Similar structure to FBGs: a periodic change to the core refractive index


- Excites significantly different effects
- Modes are resonantly coupled via phase matching condition



- Core mode is coupled into cladding modes
- Cladding modes non lossless, giving attenuation bands in transmission spectrum




- Demonstrated sensitivity to strain, temperature, bend and external refractive index



Standard Phase matching condition

$$\lambda_v = \Delta (n_{cc}(\lambda) - n_{cv}(\lambda))$$


- Gives indication of responsivity by gradient

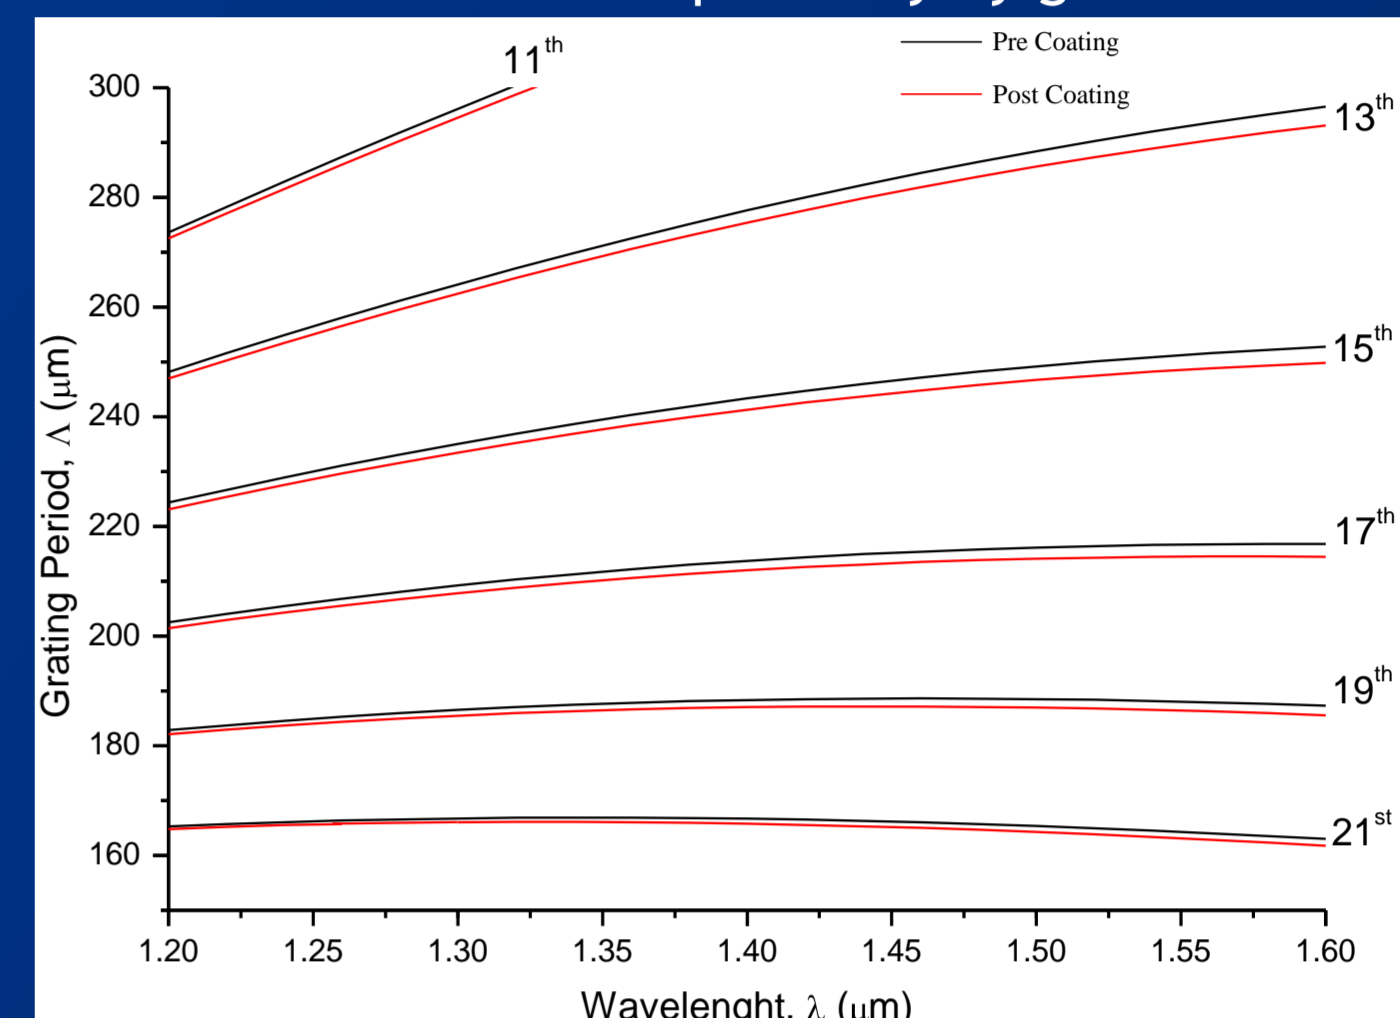

4. Modelling

Model developed at Heriot-Watt based on Erdogan*

- Model solves dispersion equations for available core and cladding modes
- Coupled mode theory then applied to determine the transmission spectrum
- Circularly symmetric 3 layer solution
- Model validated by comparing to independent CGCRI model based on matrix method

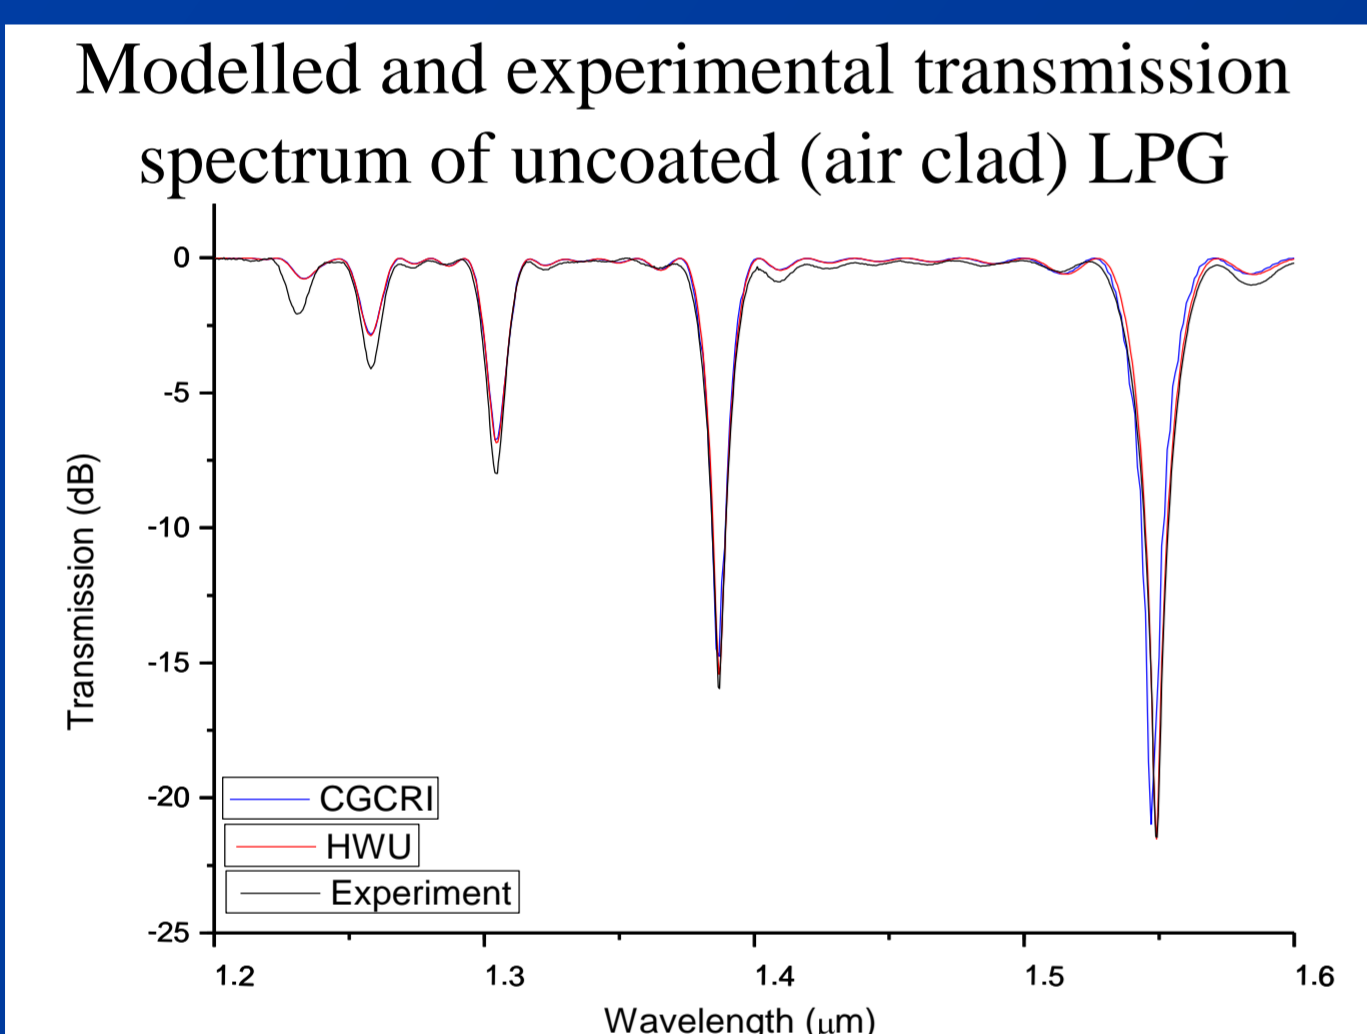


- Model accurately predicts resonant wavelengths (to within 10⁻⁶ RIU)

T. Erdogan, "Cladding-mode resonances in short- and long-period fiber grating filters," Journal of the Optical Society of America A, 14(8), 1760-1773 (1997).
T. Erdogan, "Fiber grating spectra," Journal of Lightwave Technology, 15(8), 1277-1294 (1997).
T. Erdogan, "Cladding mode resonances in short- and long-period fibre grating filters: errata," Journal of the Optical Society of America A, 17(11), 2113 (2000).

Erdogan Model not applicable to metal jacketed case

- Total internal reflection index guiding replaced by reflective layer
- External refractive index larger than cladding
- Necessary to re-evaluate Erdogan's assumptions




- Returned to the general case outlined by Tsao*
- No alteration of LPG structure
- Retain circular symmetry
- Pd refractive index determined through ellipsometry*

- Effective refractive index of cladding modes experimentally verified to remain lower than the cladding index despite metal layer

C. Tsao, [Optical fibre waveguide analysis] Oxford University Press, (1992).
R. M. Carter, P. Morrall, R. R. J. Maier et al., [Optical characterisation of RF sputter coated palladium thin films for hydrogen sensing] Spie-Int Soc Optical Engineering, Bellingham (2011).

Phase matching curves combined with couplings coefficients suggest sensitive modes


- Phase match plots indicate higher sensitivity (flatter curves) to the phase match turning point
- Higher order modes are not necessarily useful
- Necessary to determine the coupling coefficients in the presence of palladium




- Coupling coefficients remain high to the ~19th order
- Phase matching curves suggest highest sensitivity at 19th-21st order modes

Practical consideration of inscription must be taken into account

- Higher order modes give flat resonances
- Easy to miss intended resonance conditions




- Difference between pre and post coated spectrum makes inscription to exact specifications challenging
- Slightly lower order modes are preferable for manufacture, sensitivity and coupling coefficient



5. Results

Early results show small response for low order modes


- Early experiments focused on lower order modes
- Efforts made to characterise Pd thin films and LPGs separately
- 9th order shows 62pm shift to 1% H₂ (20nm feature)




- Small shift is very challenging to measure
 - Requires expensive equipment
 - Long scan times
- System highly temperature dependant
- Relatively slow response (~1hr-2hrs)
- Experiments moved on to modelling complete LPG-Pd system
 - Higher order modes identified as more attractive sensor elements

As expected higher order mode demonstrates improved response


- 15th order shows ~112pm to 1%

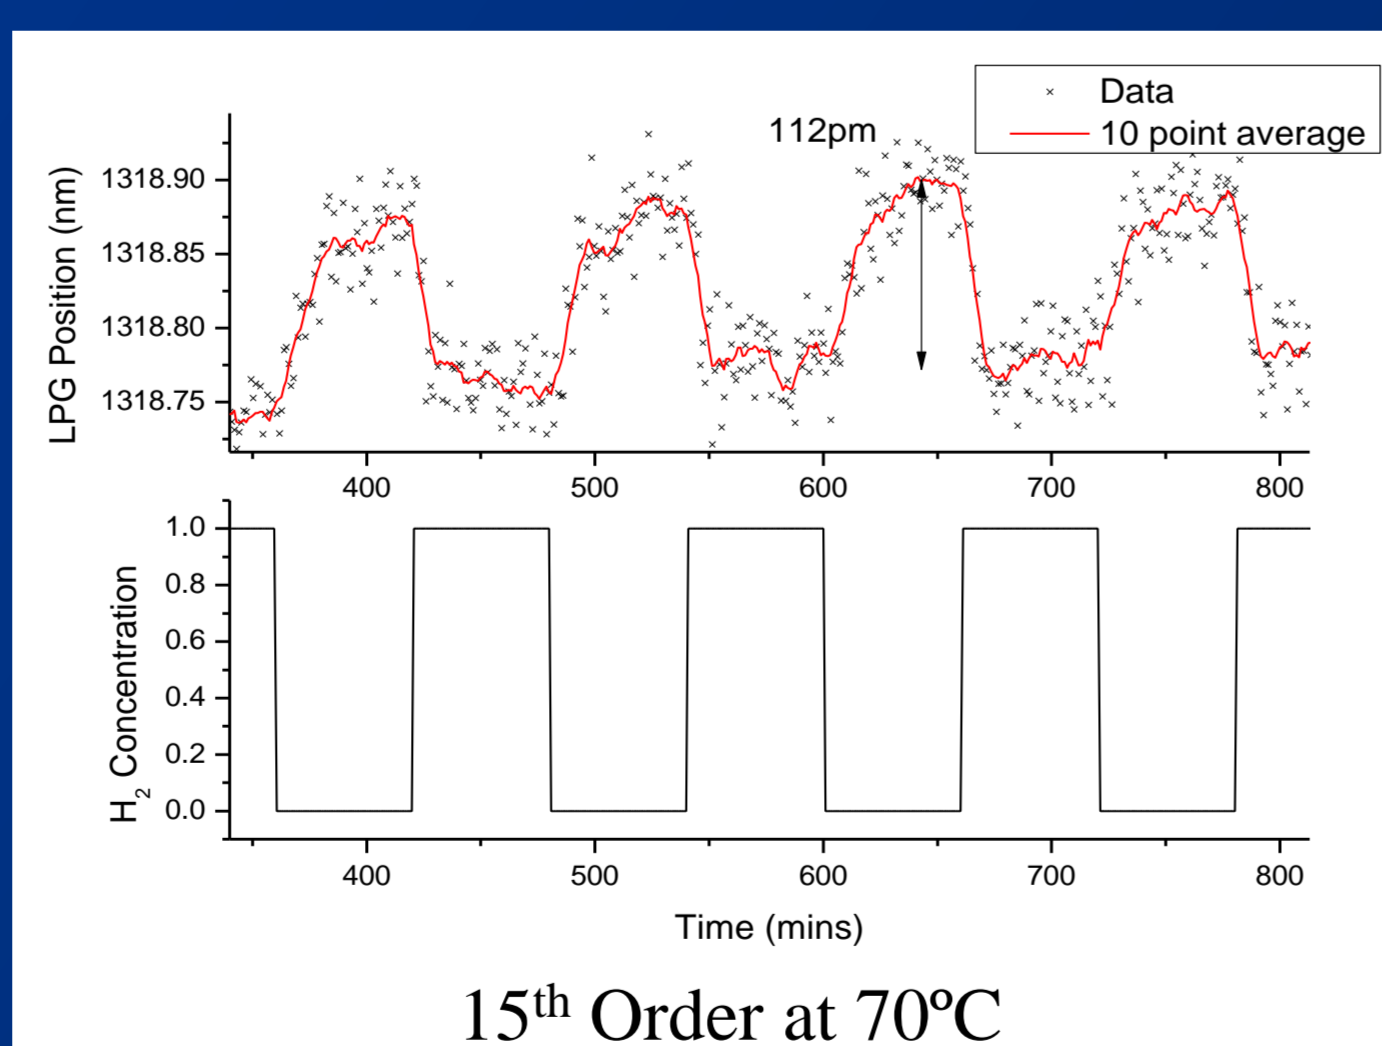


- 17th order shows ~447pm to 1%

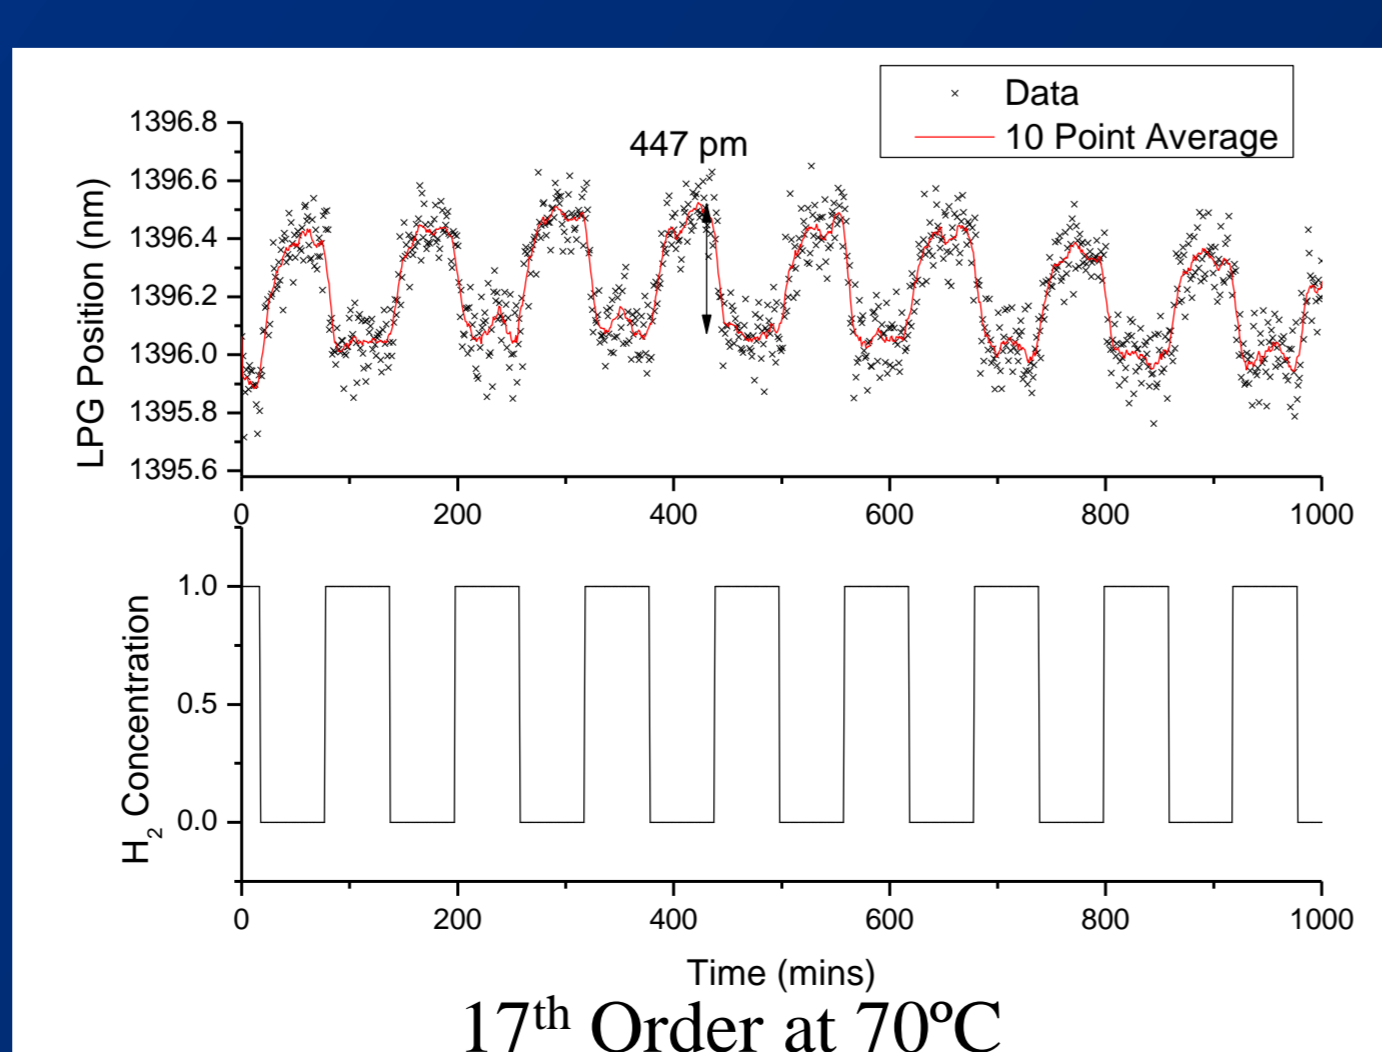

Temperature affects response



- Lower temperature gives larger but slower response
- Cycling time too short for equilibrium in this case
- Thermal noise scales with response



6. Conclusions

High mode order LPG-Pd sensors were investigated

- Analysis of the full dispersive solutions to the modelling of metal jacketed LPGs has been carried out
- High sensitivity and coupling coefficient designs have been calculated
- A range of high mode order LPG elements were manufactured by the CGCRI

High sensitivity sensors have been demonstrated

- 17th order LPG sensor has been demonstrated with 7 times responsivity of 9th order
- Scale and speed of response dependant on temperature
- Thermal sensitivity (noise) scales with sensitivity to external environment
 - No improvement in signal to noise ratio
 - Improvement in absolute response
- Thermal insensitivity/compensation requires further research

Acknowledgements

