



Heriot-Watt University
Research Gateway

Optical thickness measurement with multi-wavelength THz interferometry

Citation for published version:

Nguyen, TD, Valera Robles, JD & Moore, AJ 2014, 'Optical thickness measurement with multi-wavelength THz interferometry', *Optics and Lasers in Engineering*, vol. 61, pp. 19-22.
<https://doi.org/10.1016/j.optlaseng.2014.04.007>

Digital Object Identifier (DOI):

[10.1016/j.optlaseng.2014.04.007](https://doi.org/10.1016/j.optlaseng.2014.04.007)

Link:

[Link to publication record in Heriot-Watt Research Portal](#)

Document Version:

Publisher's PDF, also known as Version of record

Published In:

Optics and Lasers in Engineering

Publisher Rights Statement:


CC-BY

General rights

Copyright for the publications made accessible via Heriot-Watt Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

Heriot-Watt University has made every reasonable effort to ensure that the content in Heriot-Watt Research Portal complies with UK legislation. If you believe that the public display of this file breaches copyright please contact open.access@hw.ac.uk providing details, and we will remove access to the work immediately and investigate your claim.



Optical thickness measurement with multi-wavelength THz interferometry

T.D. Nguyen, J.D.R. Valera¹, A.J. Moore*

Institute of Photonics and Quantum Sciences, Heriot-Watt University, Edinburgh EH14 4AS, UK

ARTICLE INFO

Article history:

Received 19 February 2014

Received in revised form

3 April 2014

Accepted 17 April 2014

Available online 16 May 2014

Keywords:

Metrology

Interferometry

THz

Phase-step

Synthetic wavelength

ABSTRACT

We report unambiguous thickness measurement with an all-optical THz source. The optical thickness variation of a test target was measured in a Mach–Zehnder interferometer to approximately 0.5% of the illumination wavelength using an optical parametric THz laser. The frequency of the laser was continuously tuneable, enabling a synthetic wavelength to be produced by sequential illumination at discrete frequencies, thus extending the unambiguous measurement range to half the synthetic wavelength. The all-optical source provides some advantages with respect to opto-electronic and electronic sources, particularly measurement speed and resolution.

© 2014 The Authors. Published by Elsevier Ltd. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/3.0/>).

1. Introduction

The potential advantages of metrology at terahertz (THz) wavelengths are well-known. Many common non-polar materials are semi-transparent at THz wavelengths, including silicon, plastics, paper, cardboard, wood and clothing. The wavelength is long enough to avoid harmful ionizing effects but short enough to provide sub-millimetre spatial resolution for many imaging applications. Strong characteristic absorption wavelengths enable spectroscopic identification of specimens, whilst polar liquids (e.g. water) and metals are opaque.

THz time domain spectroscopy (THz-TDS) is the most widely used technique at THz wavelengths [1–3], and has been adapted for imaging [4]. Typically the opto-electronic source is a photo-conducting dipole antenna illuminated with a femtosecond (fs) laser pulse that produces a broadband THz pulse with a sub-picosecond rise time [5], [6]. Coherent detection (i.e. the amplitude and phase) of the THz pulse is achieved with a second antenna that is gated by the same fs laser via a mechanically scanned delay line. THz-TDS has been implemented for optical thickness [7] and range [8] measurements, where detection of the zero crossing of the electric field of the single-cycle pulse enables $\sim 1 \mu\text{m}$ depth resolution, determined by the positioning accuracy of the delay line. The mean output power of such systems is relatively low,

making the imaging speed slow when the spectroscopic information is not required.

The delay line can be eliminated whilst retaining coherent detection in THz-TDS. Wilk et al. [9] measured the thickness variation of a polyethylene wedge using a continuous wave THz spectrometer operating at 300 GHz based on two dipole antennas (generation and detection) both driven by two laser diodes. The detected photocurrent was recorded with and without the sample, and the thickness determined from the measured phase delay and the known refractive index. In order to measure thicknesses greater than the THz wavelength, Scheller et al. [10] used a similar system but with the dipole antennas illuminated simultaneously at three wavelengths to generate and detect three THz signals. The phase delay introduced by a polyethylene stepped wedge sample was measured for the synthetic difference frequency between the two highest THz frequencies (380 and 447 GHz). Simultaneous illumination by THz frequencies avoided the need to perform sequential phase measurements at each frequency. Zhang et al. [11] had previously introduced a synthetic difference frequency approach with traditional pulsed, broadband THz-TDS. The optical thickness of a polyethylene wedge was measured and it was noted that the noise at the composite wavelength was reduced because the noise at the constituent wavelengths was recorded simultaneously and was therefore correlated.

Electronic THz sources generally provide higher output powers. They have been used with direct detection for thickness and profile measurements, with the ultimate goal of achieving real-time imaging, although this has still not been realised to date. Hils et al. [12] used a hybrid system comprising a microelectronic Gunn oscillator operating at 600 GHz and dual coherent electro-optic

* Corresponding author.

E-mail address: a.moore@hw.ac.uk (A.J. Moore).

¹ Present address: Renishaw Plc, Research Park North, Riccarton, Edinburgh EH14 4AP, UK.

detectors. The two detectors directly compared the phase of the THz reference beam with the phase of the THz wave scattered from an object. The concept is analogous to heterodyne detection, with the fs laser triggering the electro-optic detectors acting as a local oscillator, obviating the need for mechanical scanning. Lu et al. [13] used a Gunn oscillator operating at 320 GHz launched into sub-wavelength diameter polyethylene fibre and recorded the Fabry–Perot interference intensity between a test surface and the fibre end with a Golay cell. Wang et al. [14] used two THz sources simultaneously, a Gunn diode operating at 100 GHz and a backward wave oscillator operating at 120 GHz, with a pyroelectric detector in a Michelson interferometer. One arm of the interferometer was scanned and the phase change at the synthetic wavelength with and without the target was used to calculate the optical thickness of polyethylene wedge and stepped targets.

All-optical THz sources can also provide high output powers, but at shorter wavelengths thus increasing the resolution. Each type of optical THz source has particular advantages and disadvantages, concerning output power, room-temperature operation, cost and wavelength tunability [15]. The only all-optical THz source used for thickness measurement to date was reported by Wang et al. [16] who used an optically-pumped far-infrared laser operating at 2.52 THz. The interference intensity from a Michelson interferometer was recorded with a Golay cell and the optical thickness measured at discrete points for a polyethylene wedge. The depth was determined from the known refractive index, but the absolute depth of step heights that exceeded the THz wavelength could not be calculated.

In this paper we demonstrate the first, to the best of our knowledge, unambiguous thickness measurement with an all-optical THz source. We used an optical parametric THz laser that is continuously tuneable over a large frequency range at room temperature and has a reasonably narrow-bandwidth. The all-optical source enabled direct detection that reduces the measurement time compared to opto-electronic sources, and does not require the specimen to be placed in a chamber with a dry atmosphere. It operates at a shorter wavelength than electronic sources thus increasing the resolution. Tuning this source is considerably easier than for a far-infrared laser, enabling the absorption lines of atmospheric water vapour to be avoided and sequential illumination at discrete THz frequencies to produce a synthetic wavelength for unambiguous thickness measurement.

2. Theory

The intensity I recorded by a detector at position (x) in a typical two-beam interferogram can be represented by

$$I(x) = I_0(1 + \gamma_0 \cos \phi) \quad (1)$$

where $I_0(x)$ is the bias intensity and $\gamma_0(x)$ is the visibility that depends on the relative intensities of the two beams, their coherence, and the state of polarization. When light from one of the interferometer beams undergoes a single pass through a transparent object with constant refractive index, the interference phase $\phi(x)$ between the beams changes by an amount

$$\Delta\phi_1(x) = k_1 t \Delta n_1 \quad (2)$$

where $k_1 = 2\pi/\lambda_1$ is the wave number at wavelength λ_1 , t is the geometrical thickness of the object and Δn_1 is the difference in refractive indices of the object material and the surrounding medium at wavelength λ_1 . The optical thickness $t\Delta n_1$ is ambiguous to multiples of $\lambda_1/2$. When the geometrical thickness of the object is known, measurements made with and without the object enable its refractive index to be determined from the optical thickness [17–18]. Similarly, when the refractive index is known,

the geometrical thickness can be recovered from the measured optical thickness [19]. Simultaneous measurement of the geometrical thickness and the refractive index generally require two independent techniques to be applied, for example interferometry and confocal imaging [20–21] or the use of multiple reflections within the specimen [22] and is not considered in this paper.

The change in phase produced when the object is measured at a second wavelength, λ_2 , is given by

$$\Delta\phi_2(x) = k_2 t \Delta n_2 \quad (3)$$

The phase difference between measurements at two different wavelengths can be used to extend the unambiguous range of the thickness measurement:

$$\begin{aligned} \Delta\phi_2 - \Delta\phi_1 &= 2\pi \frac{\lambda_1 - \lambda_2}{\lambda_1 \lambda_2} t \frac{\Delta n_1 + \Delta n_2}{2} \left\{ 1 - \frac{\lambda_1 + \lambda_2}{\Delta n_1 + \Delta n_2} \frac{\Delta n_1 - \Delta n_2}{\lambda_1 - \lambda_2} \right\} \\ &= 2\pi \frac{\lambda_1 - \lambda_2}{\lambda_1 \lambda_2} t \Delta n_g \end{aligned} \quad (4)$$

For dispersive media, eq. (4) contains a linear approximation to the difference of the group refractive indices Δn_g of the general form:

$$\Delta n_g = \Delta n \left\{ 1 - \frac{\lambda}{\Delta n} \frac{d(\Delta n)}{d\lambda} \right\} \quad (5)$$

For non-dispersive media $d(\Delta n)/d\lambda = 0$, in which case the group and the phase refractive index differences are equal, $\Delta n_g = \Delta n$. Then eq. (4) simplifies to

$$\Delta\phi_2 - \Delta\phi_1 = 2\pi \frac{\lambda_1 - \lambda_2}{\lambda_1 \lambda_2} t \Delta n \quad (6)$$

In both cases, the ambiguity in optical thickness $t\Delta n_g$ or $t\Delta n$ is increased to multiples of $\lambda_s/2$ where the synthetic wavelength, $\lambda_s = \lambda_1 \lambda_2 / (\lambda_1 - \lambda_2)$.

3. Experimental set-up

An intra-cavity optical parametric THz laser was used, shown schematically in Fig. 1. A Q-switched, Nd:YAG laser provided the pump-wave for the parametric oscillator. The Nd:YAG laser gain crystal was end-pumped by a fibre-coupled, quasi-continuous-wave diode laser operating at a wavelength of 808 nm. Standard quarter-wave Q-switching using an electro-optic Q-switch (QS) in combination with a quarter-wave plate ($\lambda/4$) and a linear polarizer (P) produced pump-wave pulses of typical duration 10–20 ns. The Nd:YAG laser cavity is defined by mirrors M1 and M2. The nonlinear medium Mg:LiNO₃ providing the parametric gain was located within the pump laser cavity [23], and the parametric oscillator cavity is defined by mirrors M3 and M4. A silicon prism array attached to one side of the nonlinear medium coupled the terahertz output into free-space. The laser was operated at 52 Hz pulse repetition rate, with pulses of duration 10 ns and energy of 10 nJ per pulse (peak power ~ 1 W and 0.5 μ W mean power). The spectral bandwidth was approximately 100 GHz, corresponding to a coherence length of approximately 3 mm. The THz output frequency was adjusted by rotating mirrors M3 and M4 together to modify the angle between the idler-wave cavity and the pump-wave cavity: continuous wavelength selectivity in the range 0.7–2.5 THz was achieved by changing the angle of the pump beam in

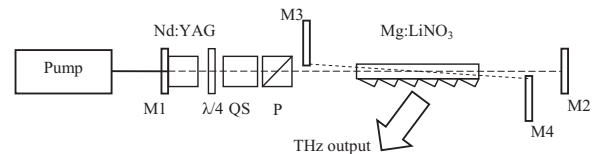


Fig. 1. Schematic of the intra-cavity optical parametric THz laser.

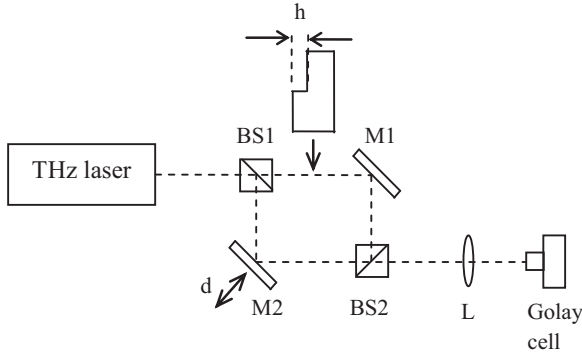


Fig. 2. Schematic of the interferometer used for thickness measurement. The test object with a step height of $h=235\ \mu\text{m}$ is shown.

the non-linear crystal. The intra-cavity position of the nonlinear medium leads to an order of magnitude reduction in the pump power required to reach oscillation threshold, accompanied by greater than an order of magnitude increase in the energies of THz pulses generated compared to conventional extra-cavity devices.

A Mach-Zehnder interferometer was constructed using the THz laser, Fig. 2. The interferometer was aligned initially with a HeNe laser (not shown), after which the THz beam was introduced. The interferometer comprised two $23\ \mu\text{m}$ thick Mylar sheet beam splitters (BS1 and BS2) and gold-coated mirrors (M1 and M2). The THz beam diameter in the interferometer was approximately 10 mm, which was reduced to 2 mm on a Golay cell detector (Tydex GC-1 P). The detector output voltage was filtered and amplified by a lock-in amplifier (Stanford Research Systems SR530). The reference beam mirror M2 was mounted on a linear translation stage (positional accuracy $\sim 1\ \mu\text{m}$) to change the optical path length of the reference beam. Moving M2 by distance d produced a path length change ($2d \cos \theta$), where θ is the angle of incidence of the laser beam on mirror M2. The object tested was $66 \times 108\ \text{mm}^2$ polytetrafluoroethylene (PTFE or Teflon) block of nominal thickness 5 mm. Material was milled from one-half of the block to produce a step height of $235\ \mu\text{m}$ (measured with a micrometre gauge).

4. Results and discussion

Fig. 3(a) shows phase-stepped intensities recorded at 0.9520 THz (wavelength $315.13\ \mu\text{m}$) for the ‘thin’ section of the object, i.e. milled half of the object. The phase was stepped through approximately π radians by moving mirror M2 in $10\ \mu\text{m}$ steps. Fig. 3 (b) shows the numerical differences between intensity measurements recorded at adjacent mirror positions, around the maximum and minimum fringe positions, of Fig. 3(a). The purpose of calculating the intensity differences was to determine positions of the maximum and minimum intensity, where the local intensity gradient is zero. As shown in Fig. 3(b) for the thin section of the object, linear fits were applied to the intensity differences and the fringe maximum and minimum positions were identified from zero crossing positions. The movement of mirror M2 between the fringe maximum and minimum for the thin section was $\Delta d=213.0-110.6\ \mu\text{m}=102.4\ \mu\text{m}$ corresponding to a measured wavelength of $\lambda_1=313.8\ \mu\text{m}$ for $\theta=40^\circ$, i.e. an error of 0.4% of the laser wavelength. For an ideal cosine, this linear fit method to the intensity difference of $\pm \pi/4$ rad around a maximum (or minimum) is accurate to $< 0.1\%$ for the position of the maximum (or minimum).

The object was then moved to illuminate the ‘thick’ section of the block, i.e. the non-machined half of the object. Fig. 3(a) shows the phase-stepped intensities recorded in the region of the fringe minimum only. Fig. 3(b) shows the intensity differences and the

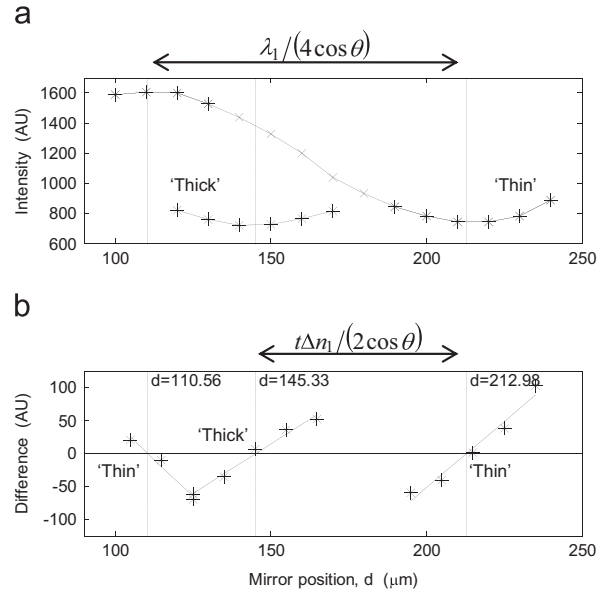


Fig. 3. (a) Phase-stepped intensity plotted against mirror position at 0.9520 THz for ‘thick’ and ‘thin’ sections of object. (b) Intensity difference between adjacent measurements and linear least squares fit in order to determine the position of fringe maximum and minima.

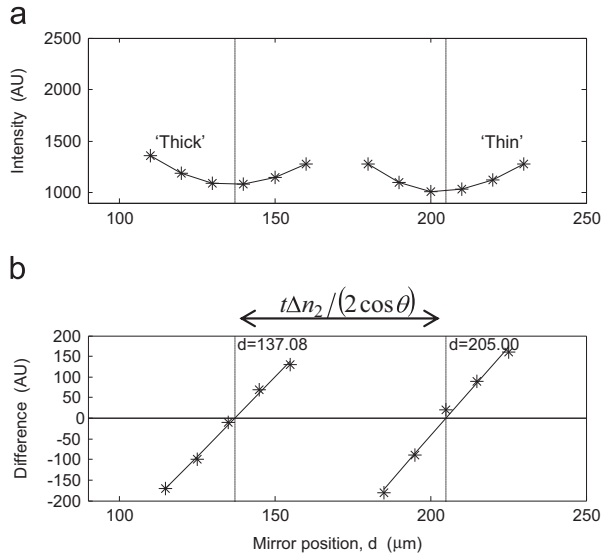


Fig. 4. (a) Phase-stepped intensity plotted against mirror position at 1.1063 THz for ‘thick’ and ‘thin’ sections of object. (b) Intensity difference between adjacent measurements and linear least squares fit in order to determine position of fringe minima.

position of the minimum identified from the linear fit. As shown in the figure, the measured change in the mirror position at the fringe minima between the thick and thin sections of the object was $\Delta d_1=213.0-145.3\ \mu\text{m}=67.7\ \mu\text{m}$, corresponding to an optical thickness $t\Delta n_1$ of $103.6\ \mu\text{m}$. Teflon is non-dispersive and has a refractive index of $n_g=n=1.445$ that varies by less than 6% over 0.2–3 THz range [24]. Therefore using $\Delta n_1=\Delta n=0.445$ for the object in air, the measured geometrical thickness of the step height was $232.9\ \mu\text{m}$, i.e. difference of 0.7% of the laser wavelength compared to the micrometre measurement. Clearly the measurement is ambiguous to multiples of half the THz wavelength.

The measurement was repeated with the laser tuned to 1.1063 THz ($\lambda_2=271.14\ \mu\text{m}$). Fig. 4(a) shows the phase-stepped intensities recorded in the region of the fringe minima for the thick and thin sections of the object. Fig. 4(b) shows the positions

of the fringe minima determined from the intensity difference. As shown in the figure, the measured change in the mirror position at the fringe minimum between the thick and thin sections of the object was $\Delta d_2 = 67.9 \mu\text{m}$, corresponding to an optical thickness $t\Delta n_2$ of $104.1 \mu\text{m}$. Therefore the measured geometrical thickness of the step height was $233.8 \mu\text{m}$, i.e. difference of 0.4% of the THz wavelength compared to the micrometre measurement. Again, this measurement is ambiguous to multiples of half the THz wavelength.

The phase differences $\Delta\phi_1$ and $\Delta\phi_2$ due to the step height can be calculated from the optical thicknesses $t\Delta n_1$ and $t\Delta n_2$ at each illumination wavelength, respectively, eqs. (2) and (3). Hence eq. (6) can be used to determine the measured step height from the synthetic wavelength ($\lambda_s = 1942.4 \mu\text{m}$) to be $239.8 \mu\text{m}$. The synthetic wavelength in measurement is 'coarse' because it magnifies the noise in the phase measured at each wavelength by the same factor as the magnification of the wavelengths. It is more accurate to divide the synthetic wavelength step height into integer multiples of one of the wavelengths, for example λ_1 , and add that number of integer wavelengths to the λ_1 measurement. For the current example, the synthetic wavelength demonstrates unambiguously that no correction is required to the measured optical thickness at either of the individual wavelengths. The unambiguous measurement range of the optical thickness has been extended to half the synthetic wavelength.

5. Conclusions

An intra-cavity optical parametric THz laser was used to measure the optical thickness variation of a test target in the Mach-Zehnder interferometer. The output frequency of the laser was tuned to 0.9520 and 1.1063 THz in order to generate a synthetic wavelength and the unambiguous measurement range was extended to seven wavelengths. An accuracy of approximately 0.5% of the THz wavelength was achieved over the extended measurement range for the step height. These are the first unambiguous thickness measurements with an all-optical THz source, to the best of our knowledge. The optical parametric THz laser enabled direct detection to reduce the measurement time compared to opto-electronic sources, and does not require the specimen to be placed in a chamber with a dry atmosphere. It operates at a shorter wavelength than electronic sources thus increasing the resolution. Tuning the optical parametric THz laser was straightforward enabling the absorption lines of atmospheric water vapour to be avoided. Having demonstrated the suitability of the source for interferometric measurements with direct detection, we are currently implementing a system for full-field measurements.

Acknowledgements

This work was supported by the Engineering and Physical Sciences Research Council (Grant number EP/F02553X/1). We are grateful to Nils Hempler and Graeme Malcolm from M-Squared Lasers and Jeorge Synowiec from Elliot Scientific Ltd. for use of the intra-cavity optical THz laser. We thank Malcolm Dunn and David Walsh from St. Andrews University for useful discussions. Andrew Moore acknowledges the support of AWE through its William Penney Fellowship scheme.

References

- [1] Auston DH, Cheung KP, Valdmanis JA, Kleinman DA. Cherenkov radiation from femtosecond optical pulses in electro-optic media. *Phys Rev Lett* 1984;53:1555–8.
- [2] Auston DH, Cheung KP. Coherent time-domain far-infrared spectroscopy. *J Opt Soc Am B: Opt Phys* 1985;2:606–12.
- [3] van Exter M, Fattinger C, Grischkowsky D. Terahertz time-domain spectroscopy of water vapour. *Opt Lett* 1989;14:1128–30.
- [4] Hu BB, Nuss MC. Imaging with terahertz waves. *Opt Lett* 1995;20:1716–8.
- [5] Smith PR, Auston DH, Nuss MC. Subpicosecond photoconducting dipole antennas. *IEEE J Quantum Electron* 1988;24:255–60.
- [6] Fattinger C, Grischkowsky D. Terahertz beams. *Appl Phys Lett* 1989;54:490–2.
- [7] Mittleman DM, Hunsche S, Boivin L, Nuss MC. T-ray tomography. *Opt Lett* 1997;22:904–6.
- [8] Cheville RA, Grischkowsky D. Time-domain terahertz impulse ranging studies. *Appl Phys Lett* 1995;67:1960–2.
- [9] Wilk R, Breitfeld F, Mikulics M, Koch M. Continuous wave terahertz spectrometer as a noncontact thickness measuring device. *Appl Opt* 2008;47:3023–6.
- [10] Scheller M, Baaske K, Koch M. Multifrequency continuous wave terahertz spectroscopy for absolute thickness determination. *Appl Phys Lett* 2010;96:151112.
- [11] Zhang LL, Zhang Y, Zhang CL, Zhao YJ, Liu HH. Terahertz multiwavelength phase imaging without 2π ambiguity. *Opt Lett* 2006;31:3668–70.
- [12] Hils B, Thomson MD, Loffler T, von Spiegel W, am Weg C, Roskos HG, et al. Terahertz profilometry at 600 GHz with $0.5 \mu\text{m}$ depth resolution. *Opt Express* 2008;16:11289–93.
- [13] Lu JY, Kuo CC, Chiu CM, Chen HW, Hwang YJ, Pan CL, et al. THz interferometric imaging using subwavelength plastic fiber based THz endoscopes. *Opt Express* 2008;16:2494–501.
- [14] Wang XK, Hou L, Zhang Y. Continuous-wave terahertz interferometry with multiwavelength phase unwrapping. *Appl Opt* 2010;49:5095–102.
- [15] Koch M. The search continues for efficient terahertz sources. *Laser Focus World* 2005;1 (November).
- [16] Wang YX, Zhao ZR, Chen ZQ, Zhang L, Kang KJ, Deng JK. Continuous-wave terahertz phase imaging using a far-infrared laser interferometer. *Appl Opt* 2011;50:6452–60.
- [17] Chamberlain JE, Gibbs JE, Gebbie HA. Refractometry in the far infra-red using a two-beam interferometer. *Nature* 1963;198:874–5.
- [18] Tearney GJ, Brezinski ME, Southern JF, Bouma BE, Hee MR, Fujimoto JG. Determination of the refractive-index of highly scattering human tissue by optical coherence tomography. *Opt Lett* 1995;20:2258–60.
- [19] Hibino, K, Kim, Y, Bitou, Y and Mitsuishi, M., Measurement of absolute optical thickness by wavelength tuning interferometer, In: Proceedings of 22nd Congress of the International Commission for Optics, 8011 (SPIE, Bellingham, WA, 2011), Article 80110B-1.
- [20] Fukano T, Yamaguchi I. Simultaneous measurement of thicknesses and refractive indices of multiple layers by a low-coherence confocal interference microscope. *Opt Lett* 1996;21:1942–4.
- [21] Ohmi M, Shiraishi T, Tajiri H, Haruna M. Simultaneous measurement of refractive index and thickness of transparent plates by low coherence interferometry. *Opt Rev* 1997;4:507–15.
- [22] DuVillaret L, Garet F, Coutaz JL. Highly precise determination of optical constants and sample thickness in terahertz time-domain spectroscopy. *Appl Opt* 1999;38:409–15.
- [23] Edwards TJ, Walsh D, Spurr MB, Rae CF, Dunn MH, Browne PG. Compact source of continuously and widely-tunable terahertz radiation. *Opt Express* 2006;14:1582–9.
- [24] Jin YS, Kim GJ, Jeon SG. Terahertz dielectric properties of polymers. *J Korean Phys Soc* 2006;49:513–7.

T.D. Nguyen received her BSc from the Vietnam National University in Hanoi in 2006. She was awarded a scholarship by the French government to study MSc in Physics and Chemistry of Solid Materials at Nancy University in France, which she received in 2008. From 2008 to 2009, she worked as a graduate research associate in CEA, France (Atomic Energy and Alternative Energies Commission). She is currently studying for her PhD in THz applications in engineering measurement.

J.D.R. Valera received his BSc in Physics from San Diego State University in 1980 and his PhD from the Optical Sciences Center at the University of Arizona in 1986. He has worked as an Associate Professor at the Norwegian Institute of Technology (NTNU) in Trondheim, JDSU in Silicon Valley, California and as an Invited Professor at the University of Gunma in Japan. In 2004 he joined Heriot Watt University as a Research Associate.

A.J. Moore received his BSc in Engineering Science and PhD in Optical Metrology from Loughborough University in 1988 and 1992, respectively. From 1992 to 1997 he worked at the Centro de Investigaciones en Optica, Mexico. He joined Heriot-Watt University in 1997 and is currently a Professor in the Institute of Photonics and Quantum Sciences. He was an EPSRC Advanced Research Fellow (October 2000 to September 2005) and is currently an AWE William Penney Fellow (August 2006 to March 2015).